

IONIX ANALYTICAL PERFORMANCES

Table of contents

1 ISE theory	1
2 Measured ions	2
3 Limits of detection	2
4 Sensitivity and Specificity	4
4. 1 : Specificity	4
4. 2 : Sensitivity	4
5 Precision	5
5. 1 : Serum mode	5
5. 2 : Urine	6
6 Accuracy	7
7 Measuring range	8
7. 1 : Serum	8
7. 2 : Urine	10
8 Interfering substances	12
9 Method comparison	12
10 Reference values	13
11 Conclusions	13

1 ISE theory

An ion-selective membrane is the key component of all potentiometric ion sensors. It establishes the preference with which the sensor responds to the analyte in the presence of various interfering ions from the sample. If ions can penetrate the boundary between two phases, then an electrochemical equilibrium will be reached, in which different potentials in the two phases are formed. If only one type of an ion can be exchanged between the two phases, then the potential difference formed between the phases is governed only by the activities of this target ion in these phases. When the mem-

brane separates two solutions of different ionic activities (α_{C1} and α_{C2}) and provided the membrane is only permeable to this single type of ion, the potential difference (E) across the membrane is described by the [Nernst equation](#):

- $E = E^\circ + RT \log (\alpha_C)/nF$,
- E = potentiel of the electrode in the measured solution
- E° = potentiel of the electrode in reference solution
- RT/nF = constant (depending of absolute temperature T)

With:

- R is [Ideal gas constant](#), equal to $8,3144 \text{ J} \cdot \text{mol}^{-1} \cdot \text{K}^{-1}$
- T is the temperature in [kelvin](#)
- F is the [Faraday constant](#), equal to $96485 \text{ C} \cdot \text{mol}^{-1}$
- n is the number of electrons transfered in the half reaction
- α ionic [activity](#) depends of ionic strength. a is the chemical activity for the relevant species, where a_{Red} is the activity of the reduced form and a_{Ox} is the activity of the oxidized form. Similarly to equilibrium constants, activities are always measured with respect to the standard state (1 mol/L for solutes, 1 atm for gases). The activity of species x, a_X , can be related to the physical concentrations c_X via $a_X = \gamma_X c_X$, where γ_X is the activity coefficient of species X. Because activity coefficients tend to unity at low concentrations, activities in the Nernst equation are frequently replaced by simple concentrations.

So the Nernst equation can be simplified as:

$$E = \text{const} + S \cdot \log (C).$$

S, the Slope is equal to 59 mV/decade at 25°C when $n = 1$ (pH, Na^+ , K^+ , Li^+), -59 when $n = -1$ (Cl^-), and 30 when $n = 2$ (Ca^{++}).

2 Measured ions

Sodium, Potassium, Chloride, ionized Calcium, pH and Lithium with ion specific electrodes. Total CO_2 (bicarbonates and dissolved CO_2) is measured with a barometer.

The pH is measured only for the standardisation of i_{Ca} at 7.4

3 Limits of detection

- Limit of Blank (LoB), Limit of Detection (LoD), and Limit of Quantitation (LoQ) are terms used to describe the smallest concentration of a measure and that can be reliably measured by an analytical procedure.
- LoB is the highest apparent analyte concentration expected to be found when replicates of a blank sample containing no analyte are tested.
- $\text{LoB} = \text{mean blank} + 1.645(\text{SD blank})$
- LoD is the lowest analyte concentration likely to be reliably distinguished from the LoB and at which detection is feasible.
- $\text{LoD} = \text{LoB} + 3\text{SD blank}$
- LoQ is the lowest concentration at which the analyte can not only be reliably detected but at which some predefined goals for bias and imprec-

sion are met. The LoQ may be equivalent to the LoD or it could be at a much higher concentration.

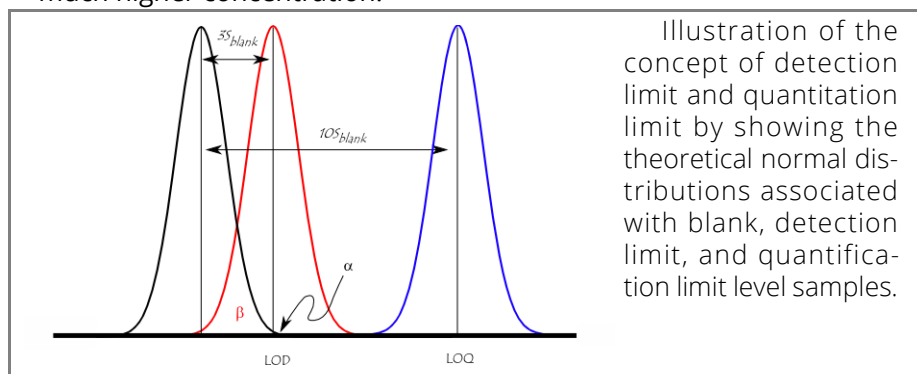


Illustration of the concept of detection limit and quantitation limit by showing the theoretical normal distributions associated with blank, detection limit, and quantification limit level samples.

For a signal at the LOD, the alpha error (probability of false positive) is small (1%). However, the beta error (probability of a false negative) is 50% for a sample that has a concentration at the LOD (red line).

For the test, the sample has been replaced by dionized water, and measured thirty times. The averages and the standard deviations are calculated, in order to determine the limits of detection and of quantification.

Table 1 : Blank, Limit of Detection and of Quantification

	Na	K	Cl	Ca	pH
	2,3	0,08	3,5	0,08	7,32
	2,6	0,08	3,7	0,08	7,3
	2,7	0,1	3,5	0,09	7,31
	2,6	0,08	3,9	0,08	7,34
	2,5	0,1	3,7	0,09	7,33
	2,9	0,08	3,7	0,09	7,37
	3,1	0,09	3,7	0,08	7,32
	2,5	0,09	3,6	0,08	7,31
	2,6	0,08	3,5	0,08	7,38
	2,6	0,1	3,8	0,08	7,26
	2,5	0,1	3,7	0,09	7,29
	2,3	0,09	3,5	0,08	7,31
	4	0,08	3,3	0,08	7,36
	2,4	0,08	3,7	0,07	7,35
	2,5	0,1	3,6	0,09	7,3
	2,5	0,08	3,9	0,08	7,29
	2,6	0,1	3,6	0,09	7,3
	2,5	0,08	3,7	0,08	7,38
	2,5	0,09	3,4	0,08	7,34
	3	0,11	3,7	0,09	7,26
	2,6	0,1	3,7	0,09	7,31
	2,4	0,09	3,7	0,08	7,33
	2,7	0,1	3,9	0,09	7,3
	2,5	0,09	3,6	0,08	7,32
	2,6	0,08	3,5	0,08	7,36
	3,5	0,11	3,8	0,1	7,21
	3,2	0,1	4,1	0,1	7,19
	2,7	0,1	3,6	0,08	7,24
	2,6	0,07	2,9	0,07	7,38
	3,4	0,08	3,9	0,08	7,09
	2,3	0,1	3,5	0,08	7,32
	2,8	0,09	3,8	0,09	7,36
	2,5	0,1	3,8	0,08	7,33
	2,4	0,08	2,4	0,07	7,45
Blank	2,69	0,09	3,61	0,08	NA
Standard deviation	0,372	0,010	0,301	0,007	NA
Limit Of Detection	3,80	0,12	4,52	0,11	NA
Limit Of Quantification	6,40	0,19	6,62	0,16	NA

4 Sensitivity and Specificity

The sensitivity is the capacity to measure a positive result (false negative), and the specificity is the capacity to measure a negative result (false positive).

4. 1 : Specificity

For all the measured ions, the probability of false positive is almost zero:

- Sodium: LOD = 3.8 mmol/L, physiological range from 135 to 145 mmol/L
- Potassium: LOD = 0.12 mmol/L, physiological range from 3.5 to 5 mmol/L
- Chloride: LOD = 4.5 mmol/L, physiological range from 90 to 110 mmol/L
- Calcium: LOD = 0.11 mmol/L, physiological range from 1.1 to 1.3 mmol/L
- For the pH these data are not available, by definition: the minimum measurement range of a pH electrode is from 2 to 12, and the physiological range is from 7.32 to 7.42

4. 2 : Sensitivity

For all the measured ions, the probability of false negative is almost zero:

- Sodium: LOQ = 6.4 mmol/L, physiological range from 135 to 145 mmol/L
- Potassium: LOQ = 0.19 mmol/L, physiological range from 3.5 to 5 mmol/L
- Chloride: LOD = 6.6 mmol/L, physiological range from 90 to 110 mmol/L
- Calcium: LOD = 0.16 mmol/L, physiological range from 1.1 to 1.3 mmol/L

5 Precision

5. 1 : Serum mode

1. Tests on water based controls:

Three controls, low, normal and high level have been tested 10 times in blood mode (serum or plasma), averages, standard deviations and CV calculated. Refer to [table 2 page, 5](#)

Table 2 : Precision on water based solutions

Code	Type	Na	K	Cl	Ca	pH	Li
ctl h	Blood	150,1	5,92	118,8	1,38	7,59	0,83
ctl h	Blood	149,8	5,94	118,8	1,38	7,59	0,83
ctl h	Blood	150,0	5,94	118,5	1,39	7,59	0,83
ctl h	Blood	150,3	5,94	118,5	1,38	7,59	0,84
ctl h	Blood	149,7	5,94	118,9	1,38	7,59	0,83
ctl h	Blood	150,1	5,91	118,5	1,39	7,59	0,83
ctl h	Blood	149,9	5,90	118,6	1,38	7,59	0,83
ctl h	Blood	149,6	5,89	118,8	1,38	7,59	0,83
ctl h	Blood	149,2	5,91	118,6	1,38	7,59	0,83
ctl h	Blood	148,6	5,92	118,3	1,38	7,58	0,83
Average		149,7	5,921	118,7	1,38	7,59	0,831
SD		0,52	0,02	0,20	0,01	0,003	0,003
CV		0,35 %	0,31 %	0,17 %	0,36 %	0,04 %	0,38 %
Mini		148,6	5,89	118,3	1,38	7,58	0,83
Maxi		150,3	5,94	118,9	1,39	7,59	0,84
ctl l	Blood	126,9	2,54	80,3	1,04	7,07	0,14
ctl l	Blood	126,7	2,53	80,3	1,04	7,07	0,14
ctl l	Blood	126,8	2,52	80,0	1,04	7,07	0,14
ctl l	Blood	126,5	2,52	80,2	1,04	7,07	0,14
ctl l	Blood	126,5	2,52	80,1	1,04	7,07	0,14
ctl l	Blood	126,6	2,54	80,0	1,04	7,07	0,15
ctl l	Blood	126,4	2,54	79,9	1,04	7,07	0,14
ctl l	Blood	126,1	2,52	80,0	1,04	7,07	0,14
ctl l	Blood	126,0	2,52	79,9	1,04	7,07	0,14
ctl l	Blood	126,3	2,52	79,5	1,04	7,06	0,14
Average		126,5	2,53	80,1	1,04	7,07	0,14
SD		0,3	0,01	0,2	0,00	0,00	0,003
CV		0,24 %	0,38 %	0,21 %	0,00 %	0,00 %	2,36 %
Mini		126,0	2,52	79,9	1,04	7,07	0,14
Maxi		126,9	2,54	80,3	1,04	7,07	0,15
ctl n	Blood	137,2	3,81	97,7	1,24	7,35	0,42
ctl n	Blood	137,1	3,81	98,0	1,24	7,35	0,42
ctl n	Blood	136,9	3,80	98,1	1,24	7,35	0,42
ctl n	Blood	137,2	3,81	97,8	1,24	7,35	0,42
ctl n	Blood	136,7	3,79	98,0	1,24	7,35	0,42
ctl n	Blood	137,1	3,80	97,8	1,24	7,35	0,42
ctl n	Blood	137,0	3,80	97,8	1,24	7,35	0,42
ctl n	Blood	136,7	3,79	97,8	1,24	7,34	0,42
ctl n	Blood	136,3	3,79	97,8	1,24	7,34	0,42
ctl n	Blood	135,6	3,78	97,6	1,23	7,34	0,42
Average		136,78	3,80	97,83	1,24	7,35	0,42
SD		0,52	0,01	0,16	0,004	0,005	0,000
CV		0,38 %	0,27 %	0,16 %	0,30 %	0,07 %	0,00 %
Mini		135,6	3,78	97,6	1,23	7,34	0,42
Maxi		137,2	3,81	98,1	1,24	7,35	0,42

2. Tests on serum

A pool of fresh serum, collected in a blood bank in dry tubes with separation gel, has been tested 31 times. Refer to [table 3 page, 5](#). For the lithium, the test has been performed on a control serum, see [table 5 page, 7](#)

Table 3 : Precision on a serum pool

Code	Na	K	Cl	Ca	pH	Li ^a
Pool 06-12	139,2	4,79	104,0	1,18	7,55	

Table 3 : Precision on a serum pool

Code	Na	K	Cl	Ca	pH	Li ^a
Pool 06-12	139,2	4,80	103,9	1,18	7,56	
Pool 06-12	139,3	4,79	104,0	1,19	7,56	
Pool 06-12	139,4	4,79	103,9	1,19	7,56	
Pool 06-12	139,3	4,80	104,1	1,18	7,57	
Pool 06-12	139,4	4,79	103,9	1,18	7,55	
Pool 06-12	139,4	4,79	104,2	1,20	7,58	
Pool 06-12	139,6	4,81	104,0	1,19	7,58	
Pool 06-12	139,5	4,80	103,9	1,19	7,57	
Pool 06-12	139,6	4,84	104,4	1,20	7,58	
Pool 06-12	139,5	4,79	104,0	1,19	7,58	
Pool 06-12	139,2	4,82	104,2	1,21	7,54	
Pool 06-12	139,3	4,84	104,3	1,21	7,55	
Pool 06-12	138,5	4,79	105,0	1,19	7,53	
Pool 06-12	139,4	4,80	104,0	1,21	7,55	
Pool 06-12	139,3	4,78	104,9	1,19	7,56	
Pool 06-12	139,4	4,83	104,2	1,21	7,53	
Pool 06-12	139,5	4,80	103,8	1,19	7,54	
Pool 06-12	139,3	4,79	104,8	1,19	7,53	0,78
Pool 06-12	139,3	4,80	103,9	1,20	7,52	0,77
Pool 06-12	139,5	4,80	104,0	1,20	7,53	0,79
Pool 06-12	138,5	4,79	104,6	1,19	7,52	0,79
Pool 06-12	139,2	4,82	104,2	1,20	7,52	0,78
Pool 06-12	138,4	4,77	104,6	1,20	7,51	0,79
Pool 06-12	139,2	4,78	104,5	1,19	7,51	0,78
Pool 06-12	139,1	4,80	103,8	1,20	7,52	0,78
Pool 06-12	139,2	4,78	103,8	1,21	7,51	0,78
Pool 06-12	138,4	4,79	104,4	1,19	7,52	0,76
Pool 06-12	139,2	4,79	104,4	1,19	7,52	0,78
Pool 06-12	139,3	4,82	103,6	1,20	7,52	0,01
Pool 06-12	139,7	4,82	104,1	1,20	7,52	1,21 %
Average	139,24	4,80	104,17	1,19	7,54	0,76
SD	0,34	0,02	0,34	0,01	0,02	0,79
CV	0,24 %	0,36 %	0,33 %	0,78 %	0,31 %	0,78
Mini	138,40	4,77	103,60	1,18	7,51	0,77
Maxi	139,70	4,84	105,00	1,21	7,58	0,79

a. Repeatability for lithium measure on a control serum

5. 2 : Urine

Tests have been performed on solutions of sodium and potassium chloride at different levels. Urine mode: sample volume is increased, no dilution. Results in [table 4 page, 6](#)

Table 4 : Precision on water based solution (urine)

Code	Na	K	Cl
repet 25	25,2	25,43	54,3
repet 25	25,9	25,52	53,2
repet 25	25,0	25,56	54,4
repet 25	25,0	25,58	53,0
repet 25	25,7	25,43	53,0
repet 25	24,9	25,52	54,4
Average	25,28	25,51	53,72
SD	0,42	0,06	0,72
CV	1,6 %	0,3 %	1,3 %
Mini	24,9	25,43	53
Maxi	25,9	25,58	54,4
repet 100	102,3	102,64	208,5
repet 100	100,5	99,84	211,7
repet 100	101,9	101,88	210,2
repet 100	98,2	101,80	210,6
repet 100	100,7	101,72	211,5
repet 100	100,3	101,57	211,6
Average	100,65	101,58	210,68
SD	1,44	0,93	1,23

Table 4 : Precision on water based solution (urine)

Code	Na	K	Cl
CV	1,4 %	0,9 %	0,6 %
Mini	98,2	99,84	208,5
Maxi	102,3	102,64	211,7
repet 150	139,4	161,09	306,4
repet 150	149,5	151,21	303,3
repet 150	154,1	149,21	306,9
repet 150	151,3	151,52	303,2
repet 150	153,1	151,25	303,0
repet 150	155,8	152,98	298,7
repet 150	153,0	148,93	304,0
repet 150	154,4	151,28	302,9
Average	153,62	150,86	303,12
SD	1,53	1,53	2,63
CV	1,0 %	1,0 %	0,9 %
Mini	151,3	148,93	298,7
Maxi	155,8	152,98	306,9

6 Accuracy

The sodium, potassium and lithium electrodes have been tested on Seronorm™ Trace Elements Serum L-1 LOT 1309438 and Seronorm™ Trace Elements Serum L-2 LOT 1309416.

The value assignment procedures has been established in accordance with the ISO 17511¹⁾ International standard using reference method procedures traceable to primary international standards.

For the lithium, the sodium and the potassium, the method is ICP-SFMS: Inductively Coupled Plasma-Sector Field Mass Spectrometry.

Table 5 : Tests on Seronorm™ Trace Elements

Time	Code	Na	K	Cl	Ca	pH	Li
11 juil. 2018 15:44	level 1	135,2	3,54	114,7	1,87	6,98	0,78
11 juil. 2018 15:43	level 1	135,0	3,54	114,1	1,89	6,99	0,77
11 juil. 2018 15:42	level 1	135,3	3,58	114,1	1,87	6,99	0,79
11 juil. 2018 15:41	level 1	135,3	3,56	114,2	1,88	6,99	0,79
11 juil. 2018 15:40	level 1	135,2	3,54	114,0	1,87	6,99	0,78
11 juil. 2018 15:39	level 1	135,1	3,55	114,2	1,87	6,99	0,79
11 juil. 2018 15:37	level 1	135,1	3,54	114,5	1,86	6,98	0,78
11 juil. 2018 15:36	level 1	134,6	3,53	114,9	1,86	6,99	0,78
11 juil. 2018 15:35	level 1	134,7	3,54	114,7	1,87	6,99	0,78
11 juil. 2018 15:34	level 1	136,3	3,58	113,3	1,81	6,98	0,76
Average		135,18	3,55	114,27	1,87	6,99	0,78
SD		0,46	0,02	0,46	0,02	0,00	0,01
CV		0,34 %	0,50 %	0,40 %	1,14 %	0,07 %	1,21 %
Mini		134,6	3,53	113,3	1,81	6,98	0,76
Maxi		136,3	3,58	114,9	1,89	6,99	0,79
Expected value (Seronorm Trace Elements Serum L-1 Lot 1309538)		127	3,2				0,758
SD		13	0,35				0,0765
Target - SD		114	2.85				0.6815
Target + SD		140	3.55				0.8345
11 juil. 2018 15:56	level 2	154,6	5,77	115,90	2,09	6,91	1,42
11 juil. 2018 15:55	level 2	154,7	5,75	115,9	2,11	6,91	1,44

1. ISO 17511. In Vitro Diagnostic Medical Devices – Measurement of quantities in samples of biological origin – Metrological traceability of values assigned to calibrators and control materials. Geneva, International Organisation for Standardization 2003.

Table 5 : Tests on Seronorm™ Trace Elements

Time	Code	Na	K	Cl	Ca	pH	Li
11 juil. 2018 15:54	level 2	152,7	5,66	117,4	2,04	6,92	1,40
11 juil. 2018 15:53	level 2	155,8	5,70	116,5	2,07	6,92	1,41
11 juil. 2018 15:51	level 2	155,9	5,72	116,5	2,09	6,91	1,42
11 juil. 2018 15:50	level 2	154,8	5,70	114,6	2,07	6,91	1,41
11 juil. 2018 15:49	level 2	154,6	5,77	115,9	2,09	6,91	1,43
11 juil. 2018 15:48	level 2	154,7	5,71	114,9	2,07	6,91	1,42
11 juil. 2018 15:47	level 2	154,3	5,69	115,8	2,09	6,91	1,42
11 juil. 2018 15:46	level 2	155,1	5,72	116,6	2,08	6,91	1,42
Average		154,72	5,72	116,00	2,08	6,91	1,42
SD		0,88	0,04	0,82	0,02	0,00	0,01
CV		0,57 %	0,62 %	0,71 %	0,91 %	0,06 %	0,78 %
Mini		152,7	5,66	114,6	2,04	6,91	1,4
Maxi		155,9	5,77	117,4	2,11	6,92	1,44
Expected value (Seronorm Trace Elements Serum L-2 Lot 1309416)		154	5,7				1,396
SD		15,5	0,55				0,1405
Target - SD		138,5	5,15				1,26
Target + SD		169,5	6,25				1,54

These tests show a good correspondance between the results obtained by the Ionix and a reference method for the sodium, the potassium and the lithium.

7 Measuring range


7. 1 : Serum

1. Sodium, potassium, chloride, calcium and pH


Table 6 : Phoenix Diagnostics electrolyte linearity test, lot 60101. Ampules have been equilibrated to room temperature during one day, and tests performed immediately after opening ampules, according to Phoenix instructions. Each level has been assayed four times.

	pH		Ca		Na		K		Cl	
	Phœnix	Ionix	Phœnix	Ionix	Phœnix	Ionix	Phœnix	Ionix	Phœnix	Ionix
Level 1	6,96	7,26	3	5,27	110	105,35	1,3	1,41	65	60,56
Level 2	7,25	7,62	2,1	2,84	130	118,86	2,3	2,16	85	80,67
Level 3	7,425	7,80	1,4	1,61	145	131,93	4,25	3,81	105	97,95
Level 4	7,575	7,97	0,95	0,94	170	143,50	6,45	5,52	120	108,18
Level 5	7,725	8,17	0,4	0,27	185	157,63	9	7,48	140	125,93


- pH response

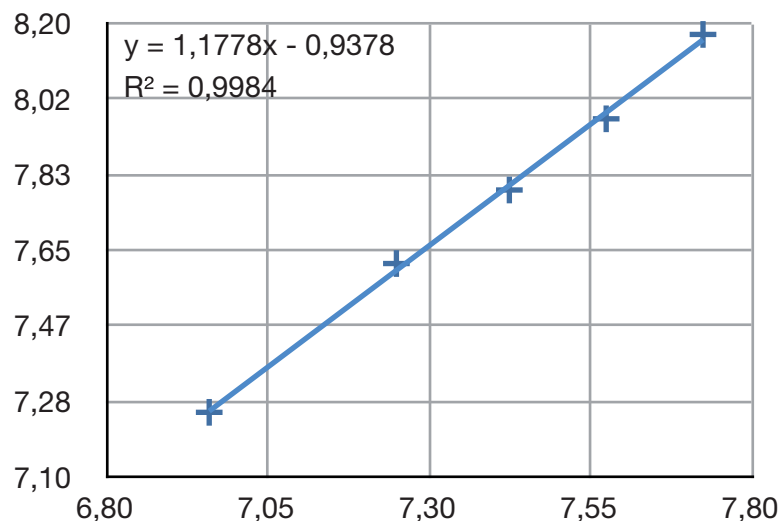


- Calcium response

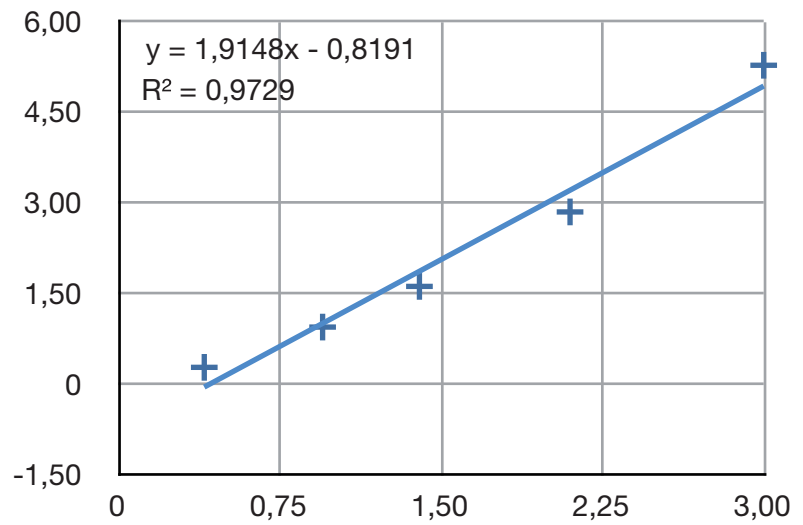


- Sodium response

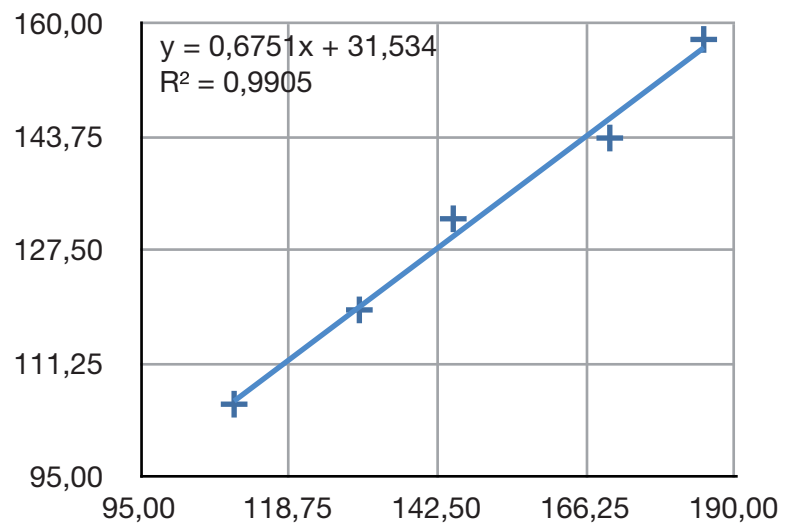

- Potassium response

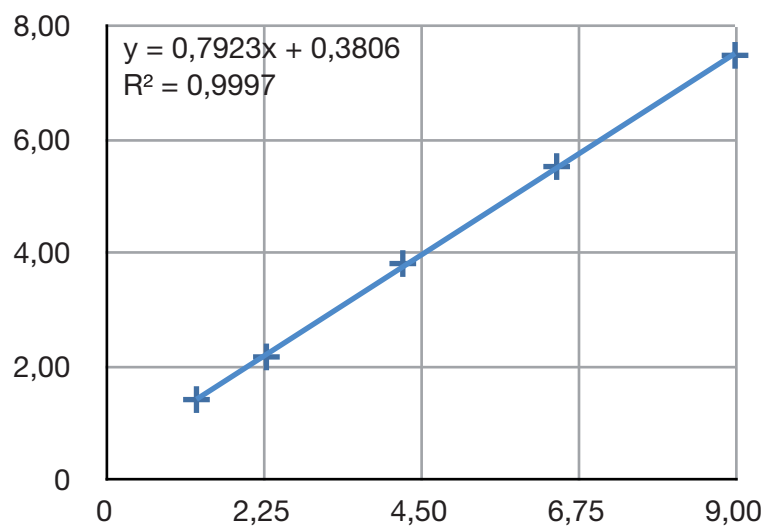


- Chloride response

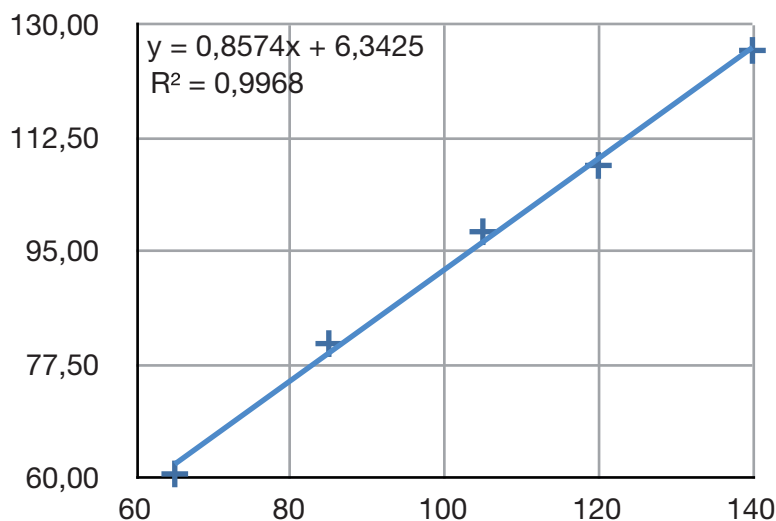

2. Lithium

A pool of serum collected on patient without lithium treatment has been prepared. A range of samples with different levels of lithium has been prepared from an heparine lithium plasma sample. The lithium concentration of this sample has been determined with a flame photometer. Dilutions by 2, 4, and 8 have been prepared, then measured three times, with the data determined above:

	Theoretical value	Measured value
Pool	0,00	0,03
Plasma/8	0,11	0,12
Plasma/4	0,21	0,21
Plasma/2	0,43	0,42
Plasma	0,85	0,81

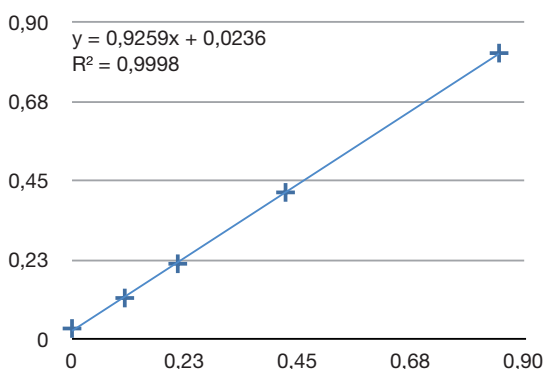

7. 2 : Urine


The linearity has been measured with a mother solution of sodium chloride (200 mmol/L) and potassium chloride (200 mmol/L) in deionized water. This mother solution has been diluted with deionized water.

Na	Na measured	K	K measured	Cl	Cl measured
0	3,23	0,00	0,11	0,00	4,97
6,25	11,30	6,25	6,15	12,50	17,10
12,5	19,33	12,50	12,49	25,00	28,83


Na	Na measured	K	K measured	Cl	Cl measured
25	33,87	25,00	25,06	50,00	51,03
50	62,67	50,00	49,58	100,00	93,20
100	121,17	100,00	97,24	200,00	167,63
150	184,20	150,00	144,04	300,00	234,80
200	240,47	200,00	192,77	400,00	299,20

For these three ions, the linearity is very good ($R^2 > 0.99$). Only a simple correction has to be applied.


- Sodium response

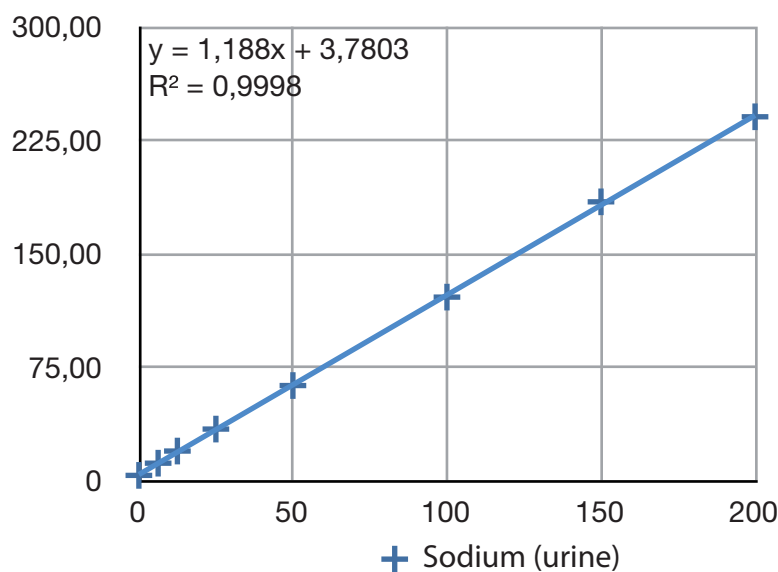

- Potassium response

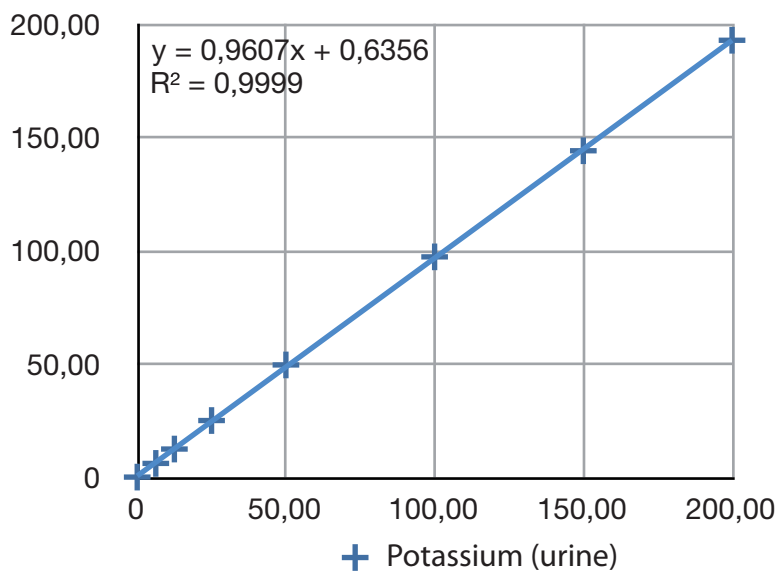

- Chloride response

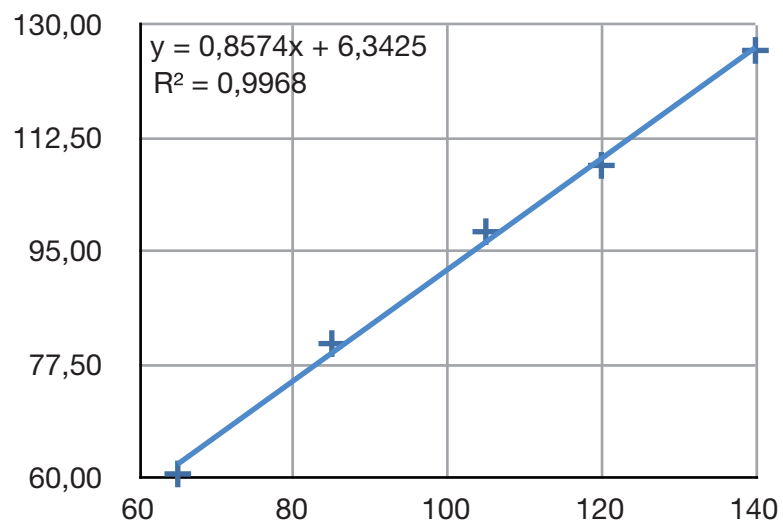

8 Interfering substances

The major interferences come from a bad preparation of the samples:

- Anticoagulants (binding effects)
- Hemolysis (sampling, storage temperature...)
- Metabolism (changes of pH)
- Evaporation

A complete chapter of the user manual describes the risks and gives some tips to avoid the major errors.

9 Method comparison

- Sodium: flame photometer. Model PHF 104 (Hycl Diagnostic), calibrator Jenway 025006, Lot FCNK517C1.
- Potassium: flame photometer. Model PHF 104 (Hycl Diagnostic), calibrator Jenway 025006, Lot FCNK517C1.
- Lithium: flame photometer. Model PHF 104 (Hycl Diagnostic), controlled with SeronormTM Trace Elements Serum L-1 LOT 1309438 and SeronormTM Trace Elements Serum L-2 LOT 1309416
- pH: pHmeter Thermoscientific, model Orion 2, sn B44156

10 Reference values

Blood	Na	K	Cl	Ca	pH ^a	Li ^b	CO ²
Low	136	3.5	98	1.07	7.32	0	23
High	145	5.1	107	1.15	7.42	1	27

a. Veinous pH at 37°C

b. The lithium is a medicament , not present in normal blood. These values represent a therapeutic range for patients under treatment.

Urine ^a	Na	K	Cl	Ca	pH
Low	40	25	95	2.5	4.6
High	220	125	250	6.2	8

a. Values only for indication. The concentrations have to be reported to the patient diuresis

11 Conclusions

Different organizations publish the desirable specifications for assays performances. From country to country the specifications can vary.

Below, the table shows the desirable biological variation specifications established by Fr. Carmen Ricos and colleagues (<https://www.westgard.com/biodatabase1.htm>).

Table 7 : Within-subject and between-subject CV values of analytes and Desirable Analytical Quality Specifications for imprecision, bias and total error

Sample	Analyte	Biological variation		Desirable specification		
		CV _i ^a	CV _g ^b	I(%) ^c	B(%) ^d	TE(%) ^e
Blood	Sodium	0.6	0.7	0.3	0.23	0.73
Urine	Sodium	28.7	16.7	14.4	8.3	32
Blood	Potassium	4.6	5.6	2.3	1.81	5.61
Urine	Potassium	24.4	22.2	12.2	8.2	28.4
Blood	Chloride	1.2	1.5	0.6	0.5	1.5
Blood	iCalcium	1.7	1.9	0.9	0.6	2.0
Blood	pH(pH units)	0.2	...	0.1

a. CV_i = within-subject biologic variation

b. CV_g = between-subject biologic variation

c. I = desirable specification for imprecision

d. B = desirable specification for inaccuracy

e. TE = desirable specification for allowable total error

The tests performed on serum on Ionix show a imprecision better than requested by Ricos.

The bias and the total error can be easily corrected by the operators if necessary.

Recommandations from other organizations are more or less strict. For more informations, refer to Westgard website (<https://www.westgard.com>). The performances of the Ionix are better than any of these recommandations.

Tests performed by	Christian Barboux	
Tests validated by	Émilie Soubielle	 <p>SFRI SAS au capital de 75 000 € N° 453 866 824 RCS Bordeaux Lez du Berganton® 33127 Saint Jean Puy - France TVA : FR 38 453 866 824 Tél. : +33 (0)5 56 68 80 50 - Fax : +33 (0)5 56 21 79 03</p>